Control H-Clk & CB-Fan in a Small System

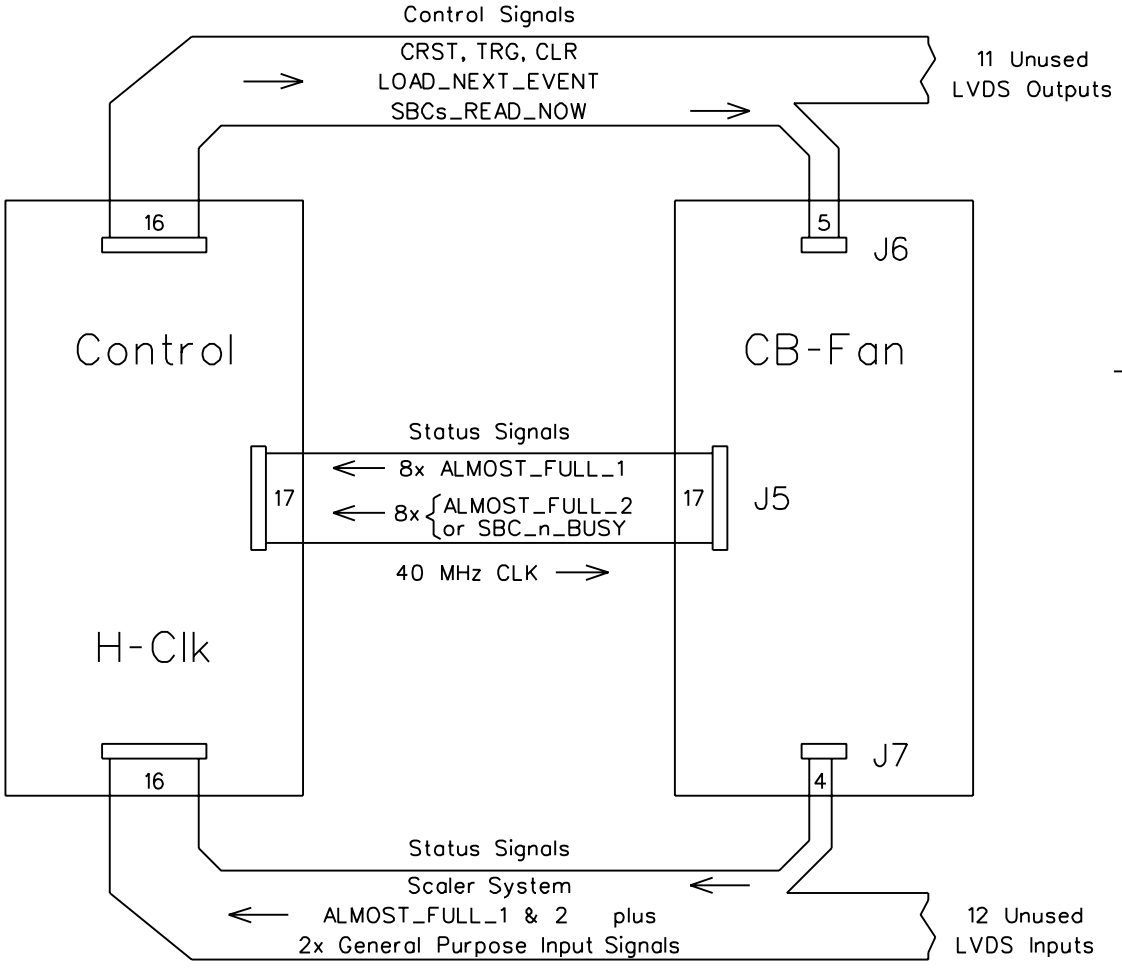

From this CB-Fan Card
there Are the Following Possible
Connections to the Trigger/DAQ System:

6x	Standard Control Buses ECL
2x	Standard Control Buses LVDS
1x	Special Control Bus for Scaler System
8x	SBCs_READ_NOW
8x	SBC_n_BUSY
1x	LOAD_NEXT_EVENT_ENABLE
1x	General Purpose Input Signal

We assume that one of the two General Purpose Input signals will carry the LOAD_NEXT_EVENT_ENABLE signal.

Rev. 26-Mar-2012