


Manually Controlled Current Source

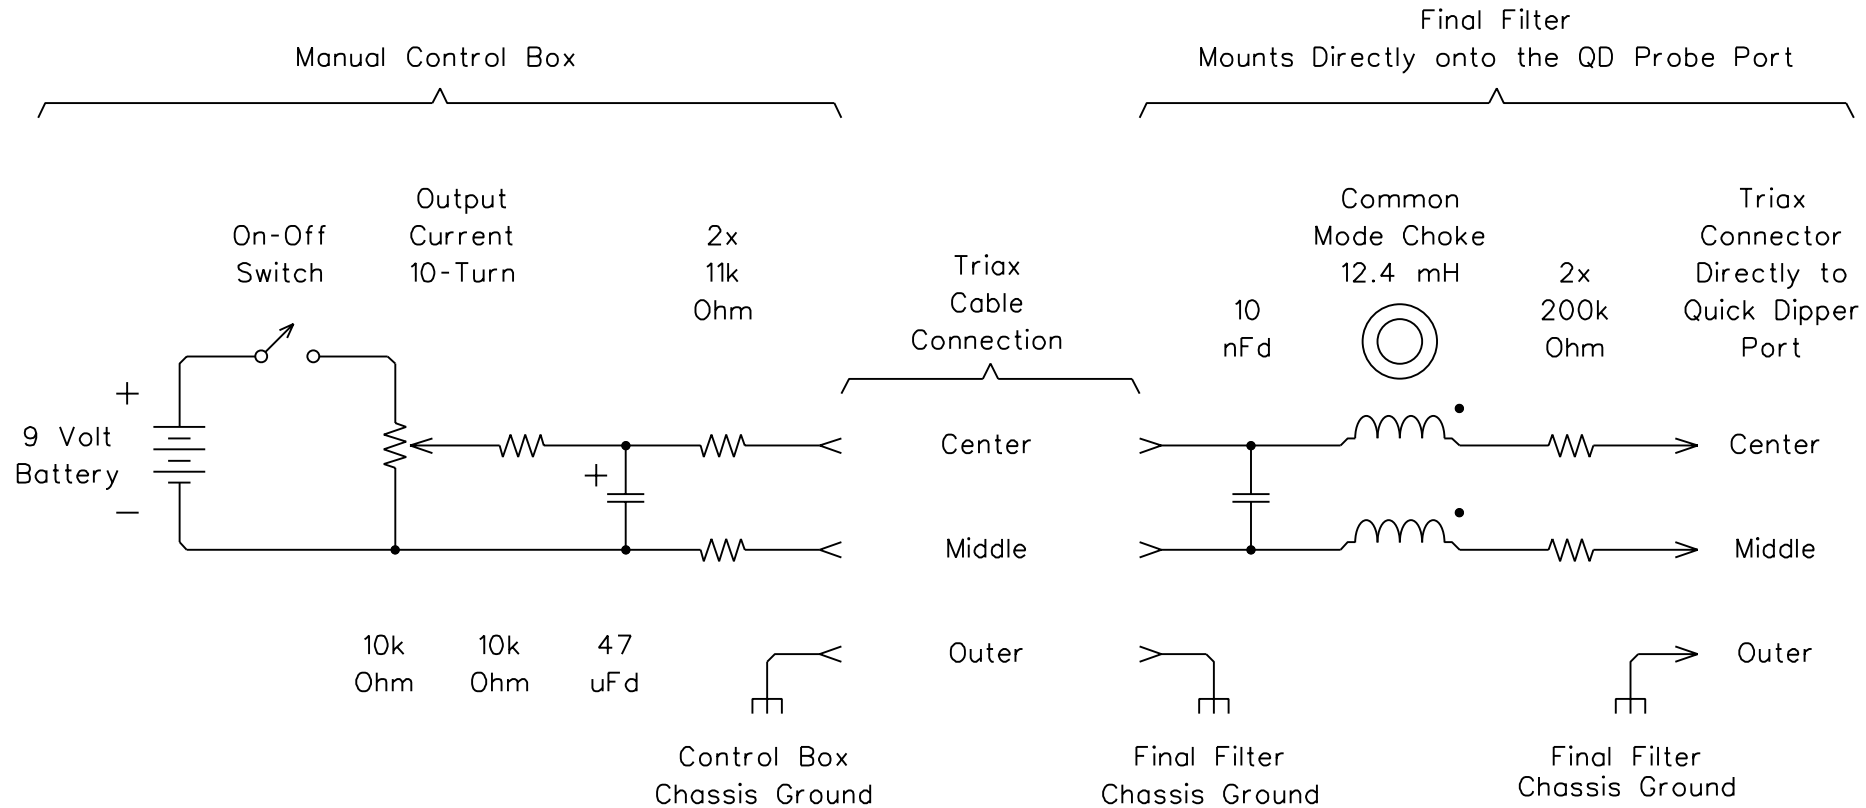

Output Current Calibration vs Dial Setting Operating with a New Battery into a 1k Ohm Load

Dial Setting	Output Current uAmp	Dial Setting	Output Current uAmp	Dial Setting	Output Current uAmp
0	0.00	350	7.60	700	15.25
50	1.08	400	8.68	750	16.35
100	2.16	450	9.78	800	17.45
150	3.25	500	10.88	850	18.56
200	4.33	550	11.96	900	19.66
250	5.43	600	13.06	950	20.80
300	6.51	650	14.15	1000	21.91